

DoseLab FractionCHECK Treatment Delivery Report

Summary: All treatment fields passed

Patient name: Doe, John

Dates treated: April 07, 2011 to April 18, 2011

Treatment machine: Childress Demo, #:23

Number of treatment log files that passed all criteria: 70

Number of treatment log files that generated a warning: 0

Number of treatment log files that failed any criteria: 0



Number of days treatments were delivered: 5

Total number of treatment fields delivered: 35

Maximum 95th percentile |error| (95P) during treatments: 0.06 mm (Pass)


Maximum leaf RMS error during treatments: 0.05 mm (Pass)

Minimum gamma passing rate during treatment: 99.3% (Pass)

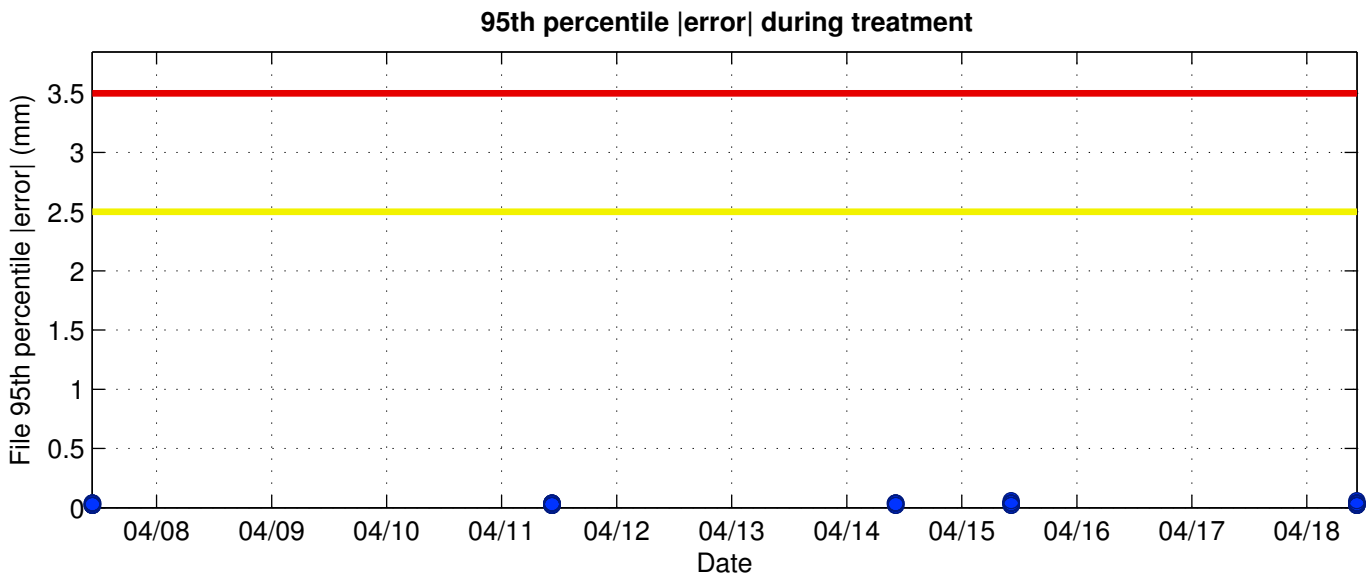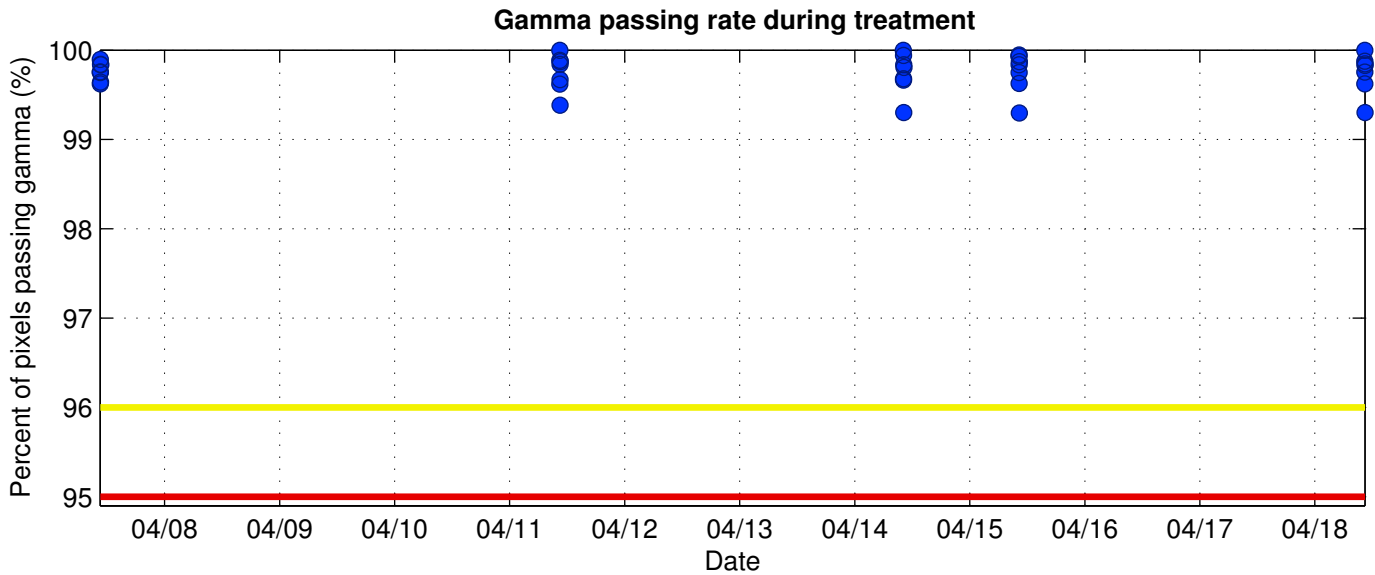


Doe, John
April 07, 2011
10:34:01 AM
Gantry: 160.0°
Collimator: 0.0°

7 segments
Time: 20.0 s
Bank A 95P: 0.02 mm
Bank B 95P: 0.02 mm
Gamma: 99.9%

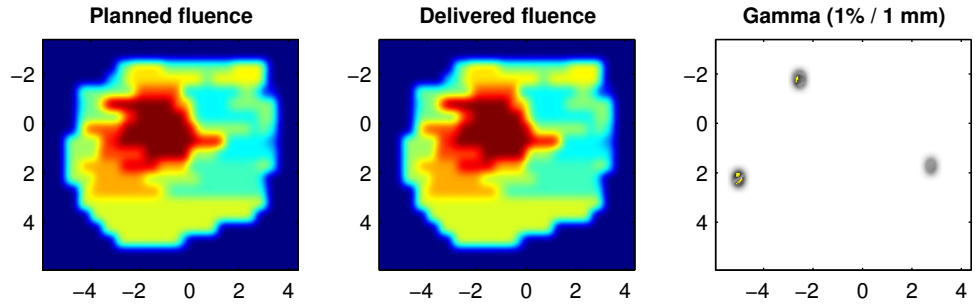


Doe, John
April 07, 2011
10:34:44 AM
Gantry: 110.1°
Collimator: 0.1°

7 segments
Time: 21.1 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.02 mm
Gamma: 99.6%

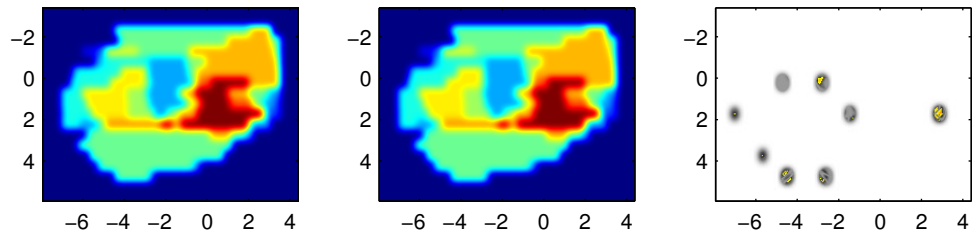


Doe, John
April 07, 2011
10:35:35 AM
Gantry: 60.0°
Collimator: 0.0°

6 segments
Time: 13.4 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.04 mm
Gamma: 99.8%

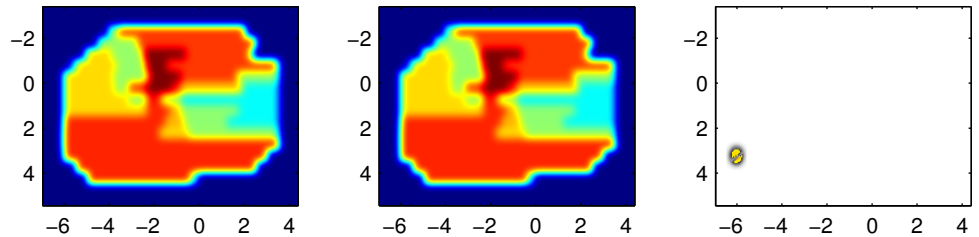

Doe, John
April 07, 2011
10:36:21 AM
Gantry: 310.0°
Collimator: 0.0°


7 segments
Time: 21.5 s
Bank A 95P: 0.02 mm
Bank B 95P: 0.02 mm
Gamma: 99.7%

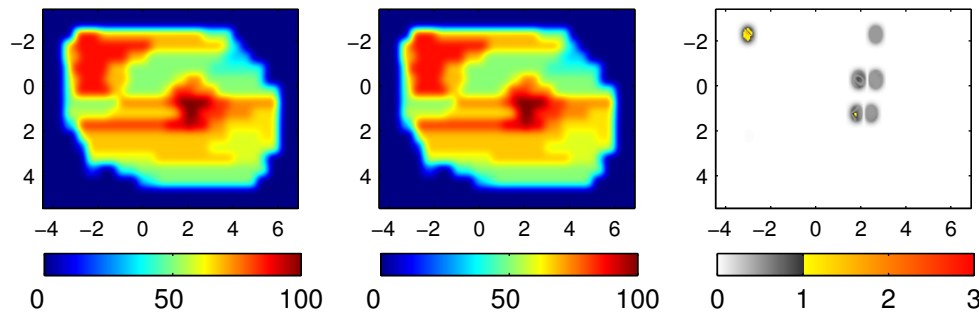

Doe, John

April 07, 2011
10:37:10 AM
Gantry: 260.0°
Collimator: 0.0°


6 segments
Time: 13.1 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.04 mm
Gamma: 99.8%

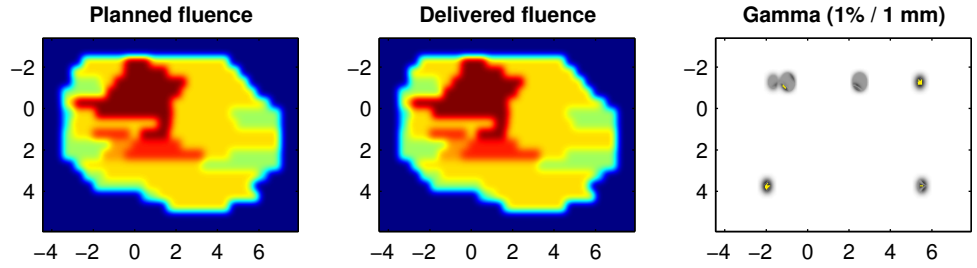

Doe, John

April 07, 2011
10:37:47 AM
Gantry: 210.0°
Collimator: 0.0°


7 segments
Time: 19.3 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.04 mm
Gamma: 99.6%

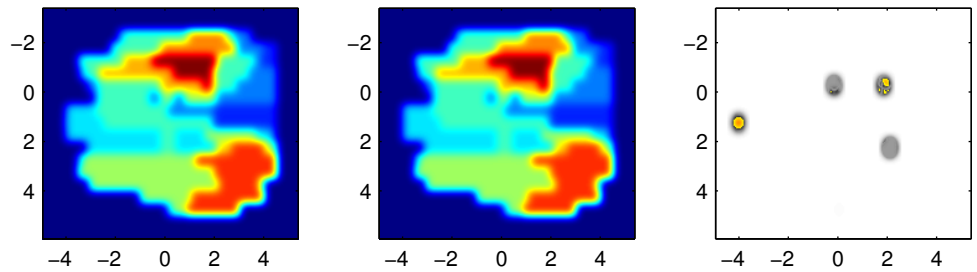

Doe, John


April 07, 2011
10:39:37 AM
Gantry: 310.0°
Collimator: 0.1°

8 segments
Time: 25.0 s
Bank A 95P: 0.02 mm
Bank B 95P: 0.04 mm
Gamma: 99.8%

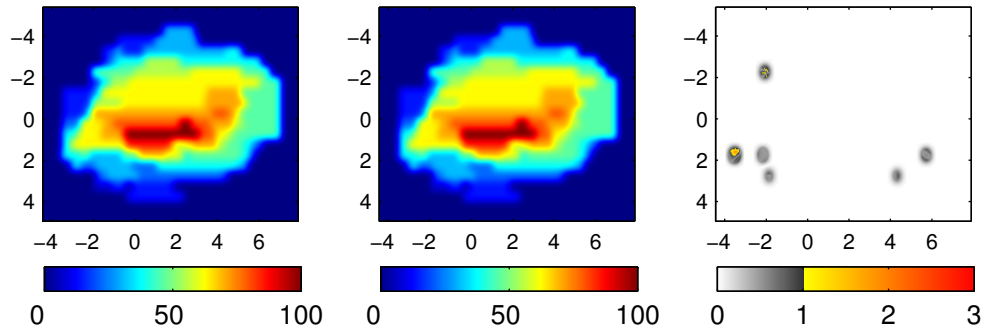


Doe, John
April 15, 2011
10:15:37 AM
Gantry: 160.0°
Collimator: 0.1°

8 segments
Time: 20.0 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.04 mm
Gamma: 99.9%

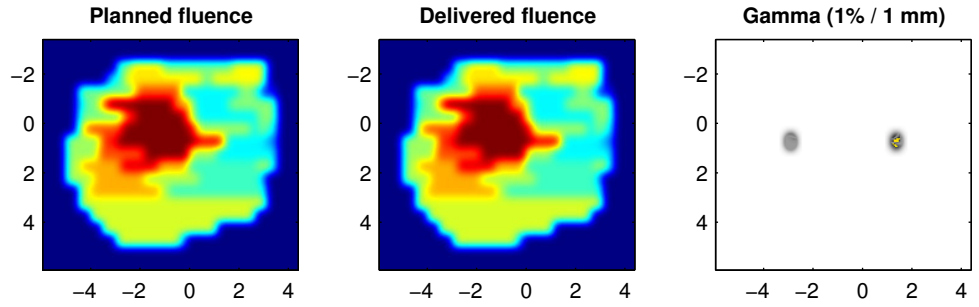


Doe, John
April 15, 2011
10:16:19 AM
Gantry: 110.0°
Collimator: 0.0°

8 segments
Time: 21.2 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.04 mm
Gamma: 99.6%

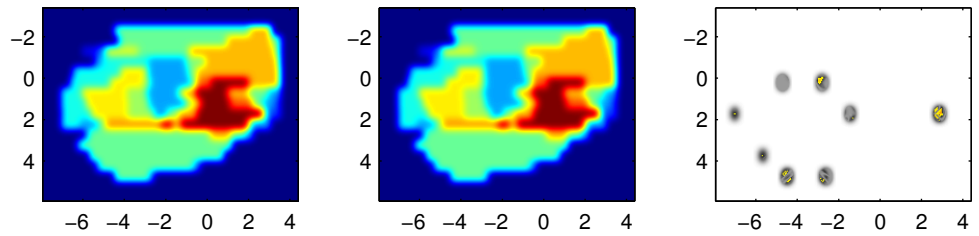


Doe, John
April 15, 2011
10:17:02 AM
Gantry: 60.0°
Collimator: 0.0°

5 segments
Time: 13.4 s
Bank A 95P: 0.06 mm
Bank B 95P: 0.04 mm
Gamma: 99.9%

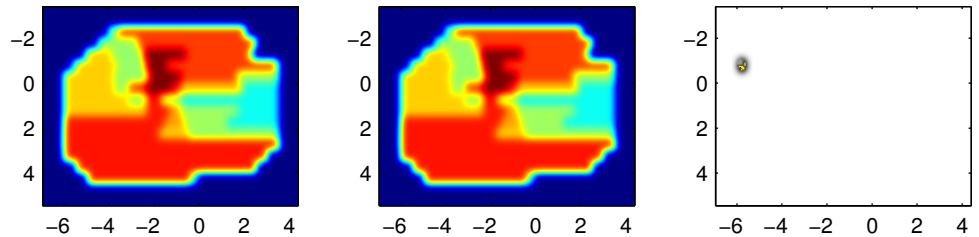

Doe, John
April 15, 2011
10:17:50 AM
Gantry: 310.0°
Collimator: 0.0°

7 segments
Time: 21.5 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.02 mm
Gamma: 99.7%

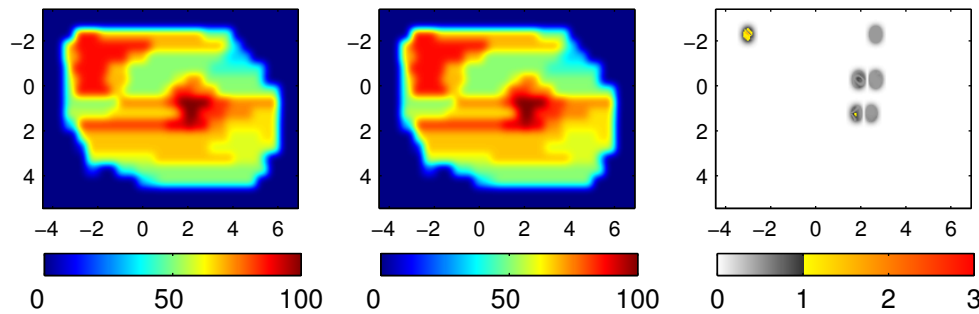

Doe, John

April 15, 2011
10:18:33 AM
Gantry: 260.0°
Collimator: 0.0°


5 segments
Time: 13.0 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.04 mm
Gamma: 99.8%



Doe, John

April 15, 2011
10:19:06 AM
Gantry: 210.0°
Collimator: 0.1°

6 segments
Time: 19.3 s
Bank A 95P: 0.04 mm
Bank B 95P: 0.04 mm
Gamma: 99.3%

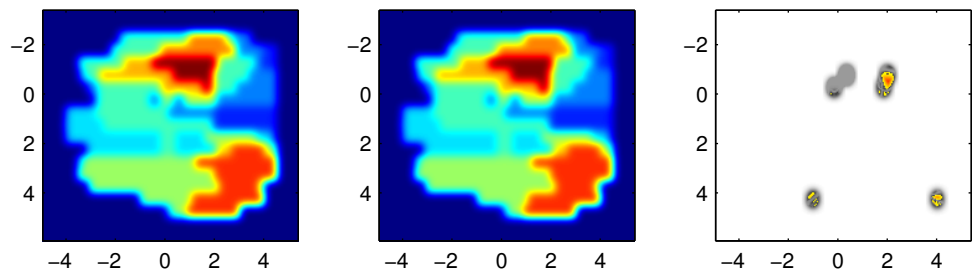

Doe, John

April 15, 2011
10:20:56 AM
Gantry: 310.0°
Collimator: 0.0°

8 segments
Time: 25.0 s
Bank A 95P: 0.02 mm
Bank B 95P: 0.02 mm
Gamma: 99.9%

